


PUSEN

Single Use Grasping Forceps

PGA



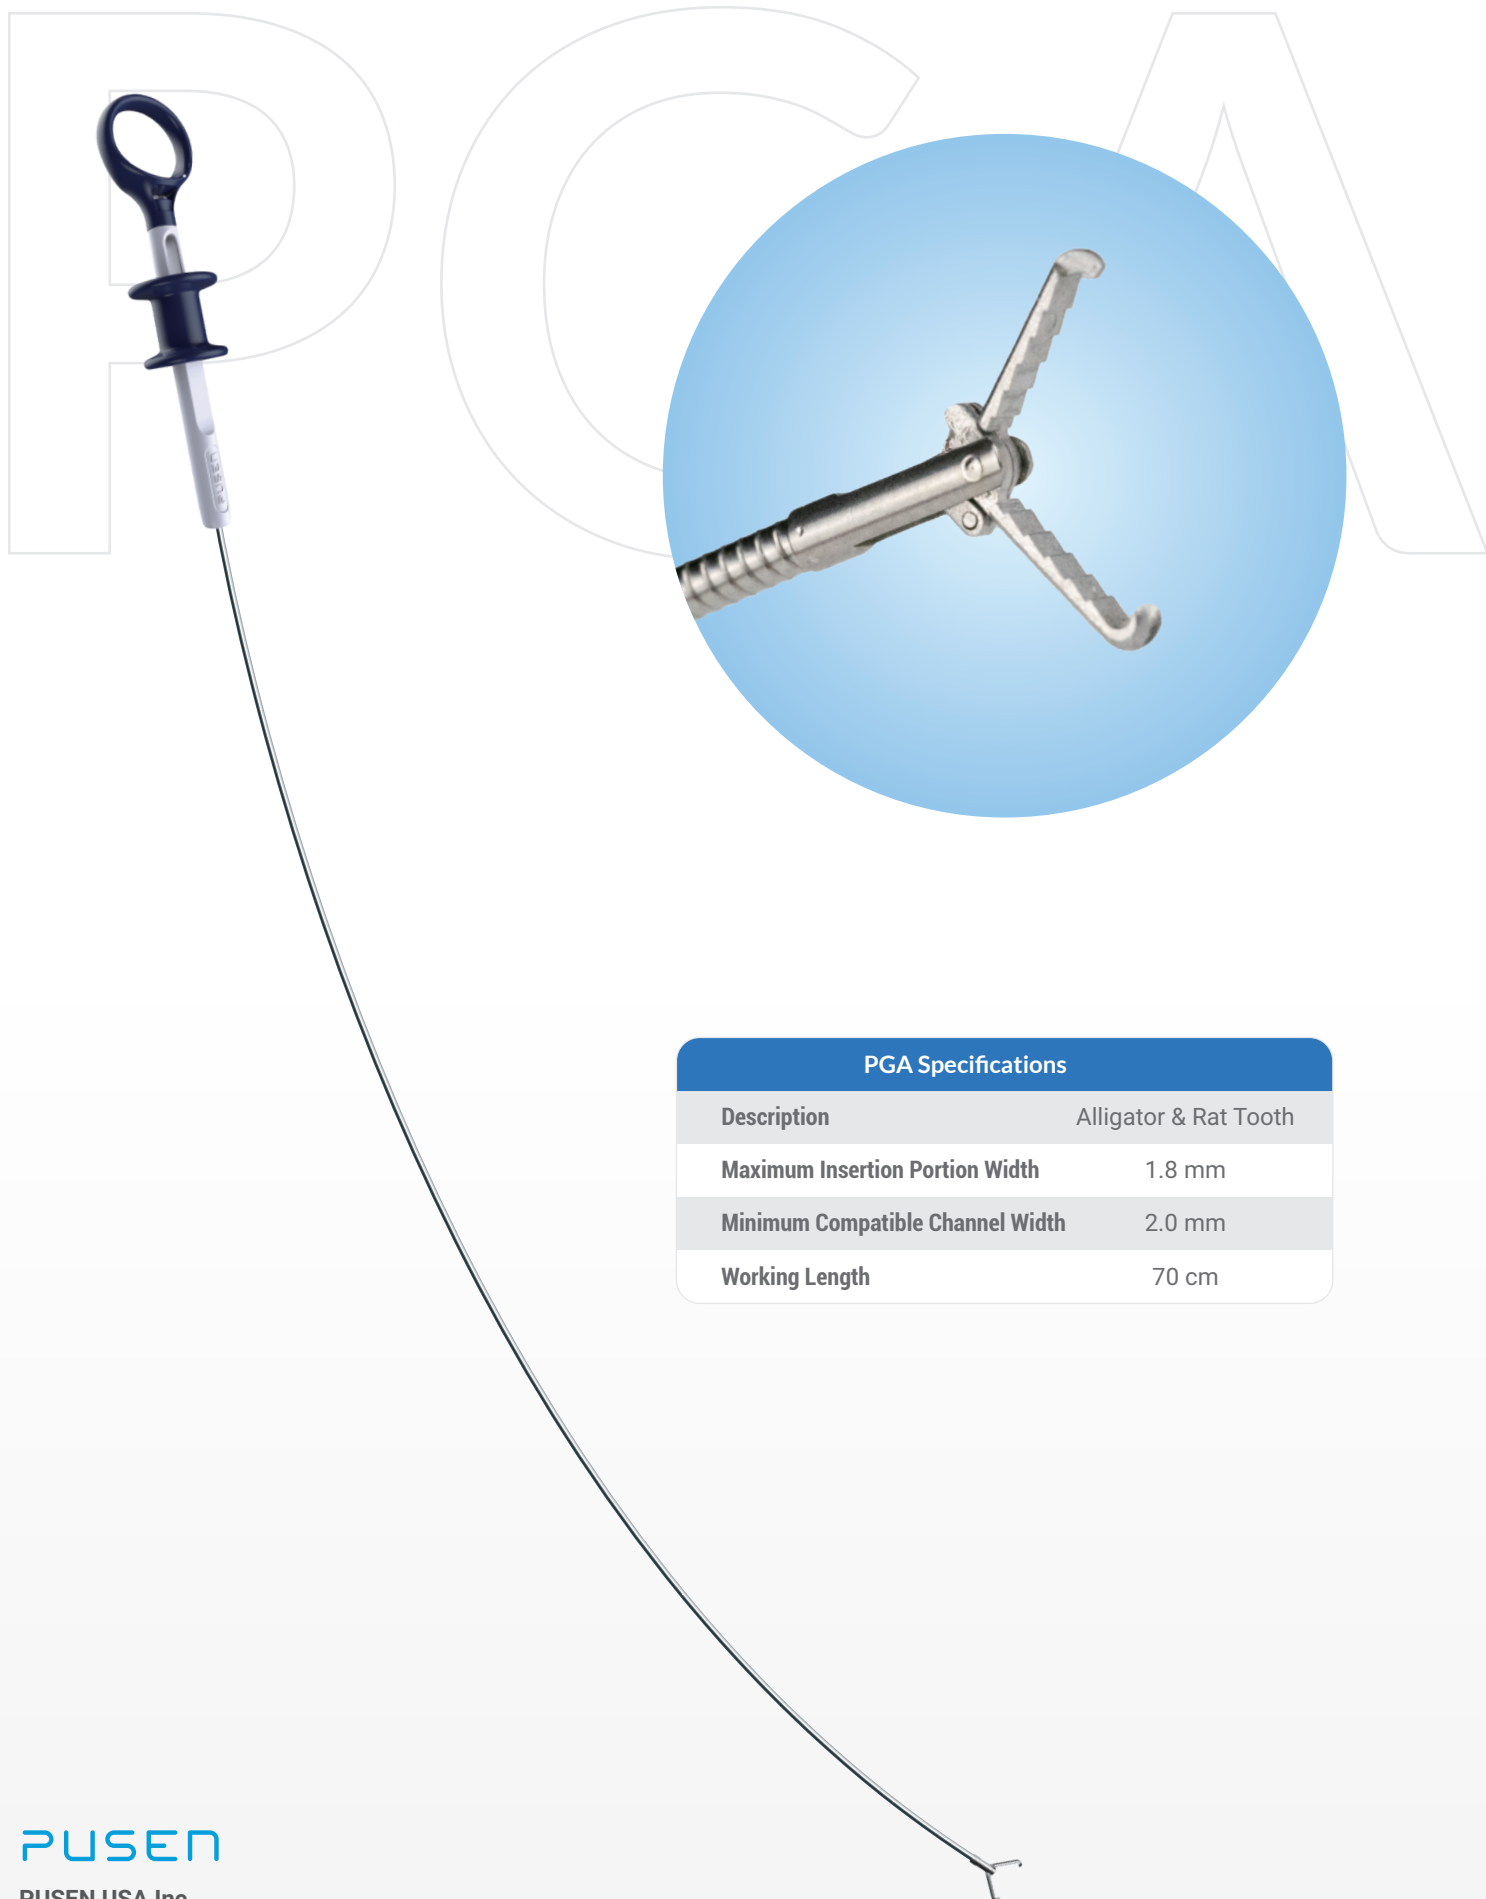

PGA Specifications	
Description	Alligator & Rat Tooth
Maximum Insertion Portion Width	1.8 mm
Minimum Compatible Channel Width	2.0 mm
Working Length	70 cm

PUSEN

PUSEN USA Inc

11340 Lakefield Dr, STE 200

Johns Creek, GA, 30097

770-527-9215

info@PUSENUA.com


Ver-US-202501

PUSEN

Single Use Biopsy Forceps

PGB



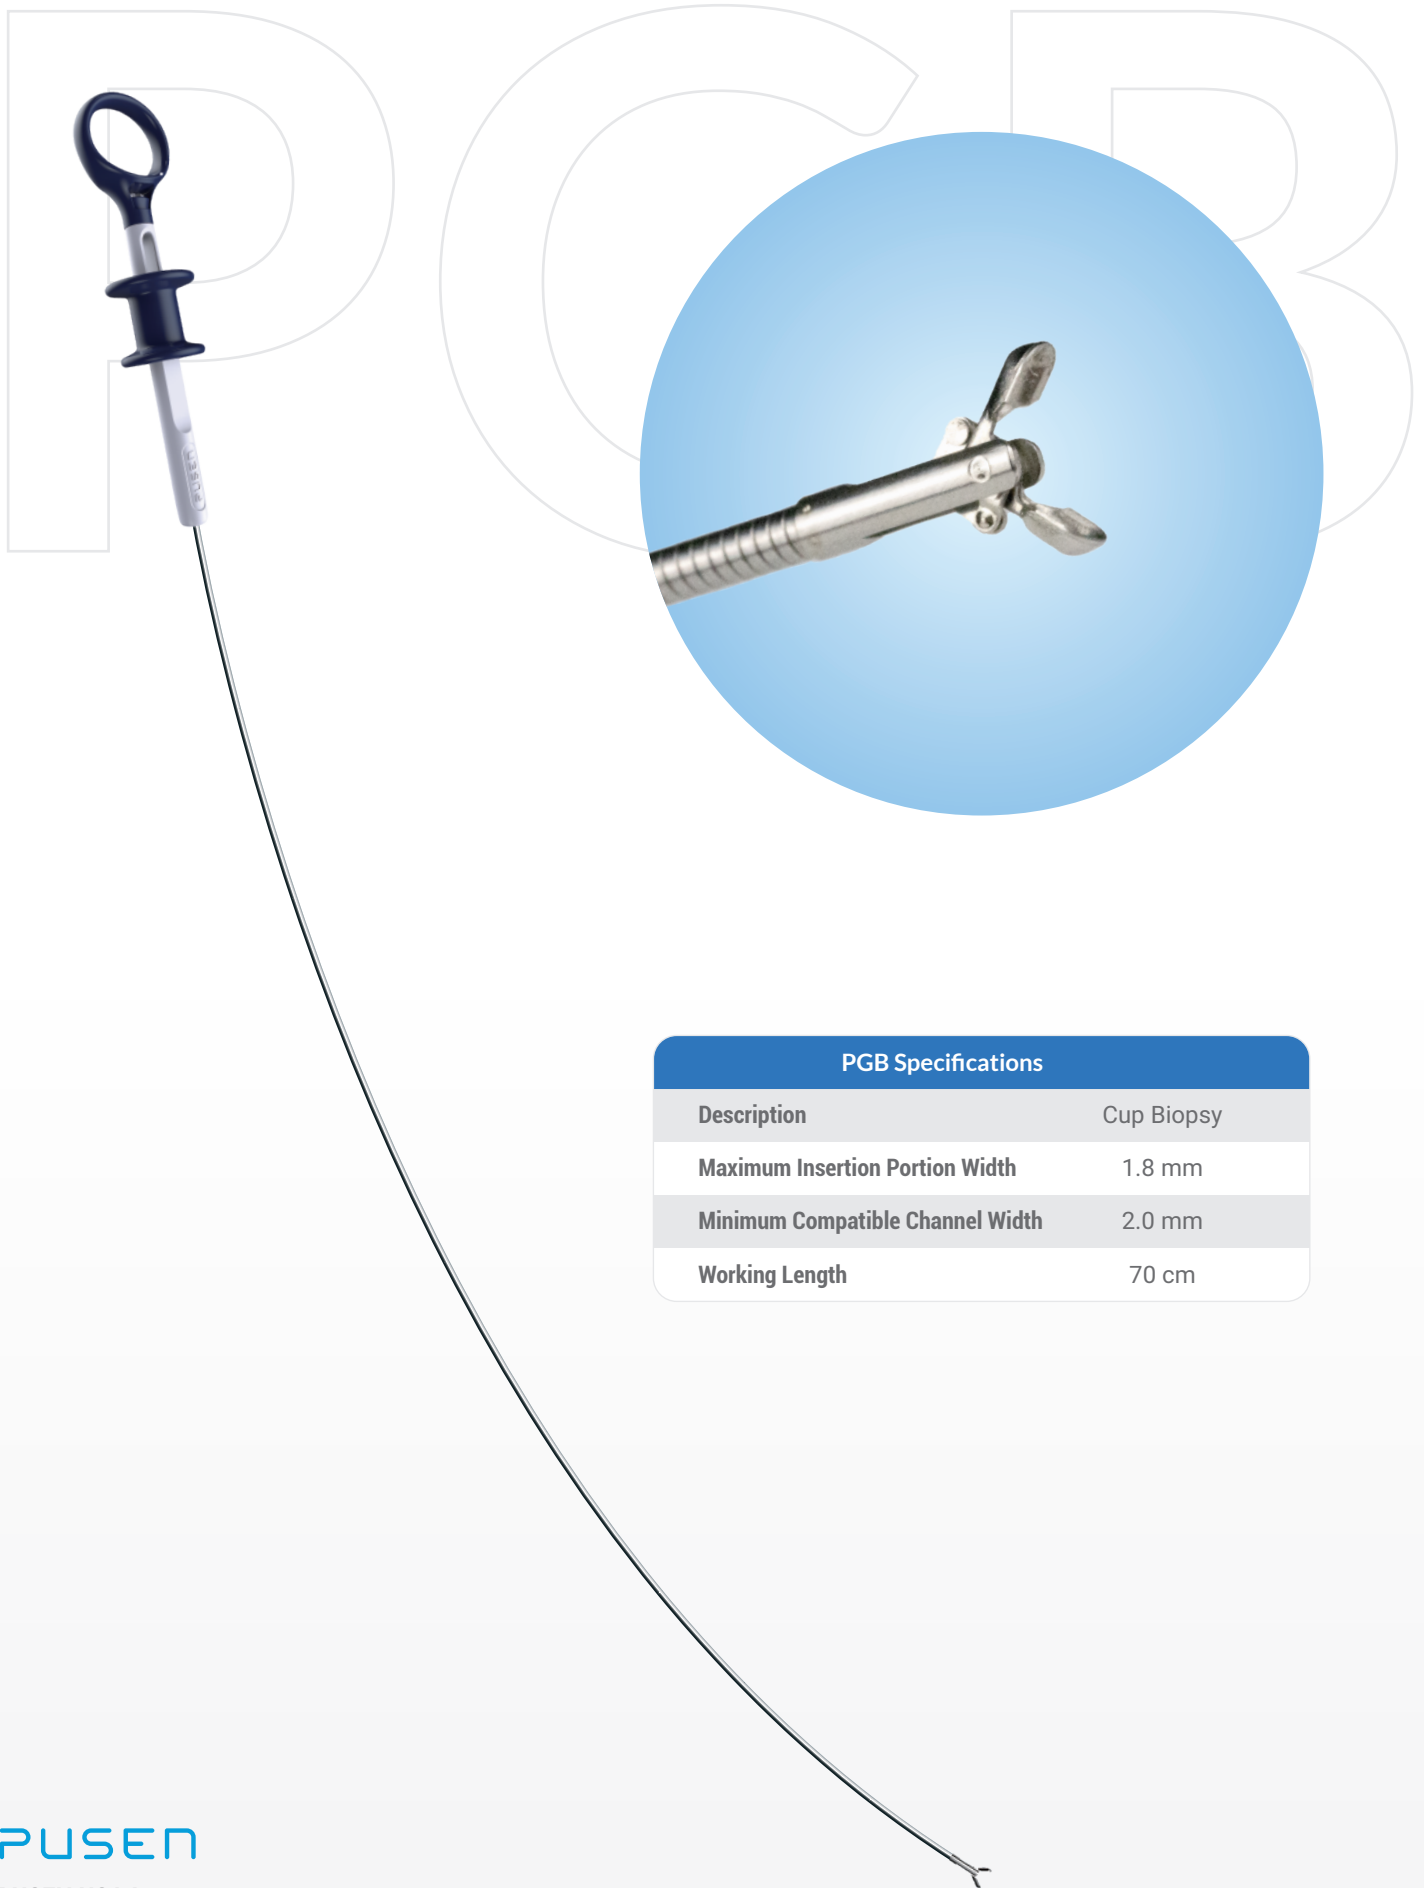

PGB Specifications

Description	Cup Biopsy
Maximum Insertion Portion Width	1.8 mm
Minimum Compatible Channel Width	2.0 mm
Working Length	70 cm

PUSEN

PUSEN USA Inc

11340 Lakefield Dr, STE 200

Johns Creek, GA, 30097

770-527-9215

info@PUSENUA.com

Ver-US-202501